

1/15

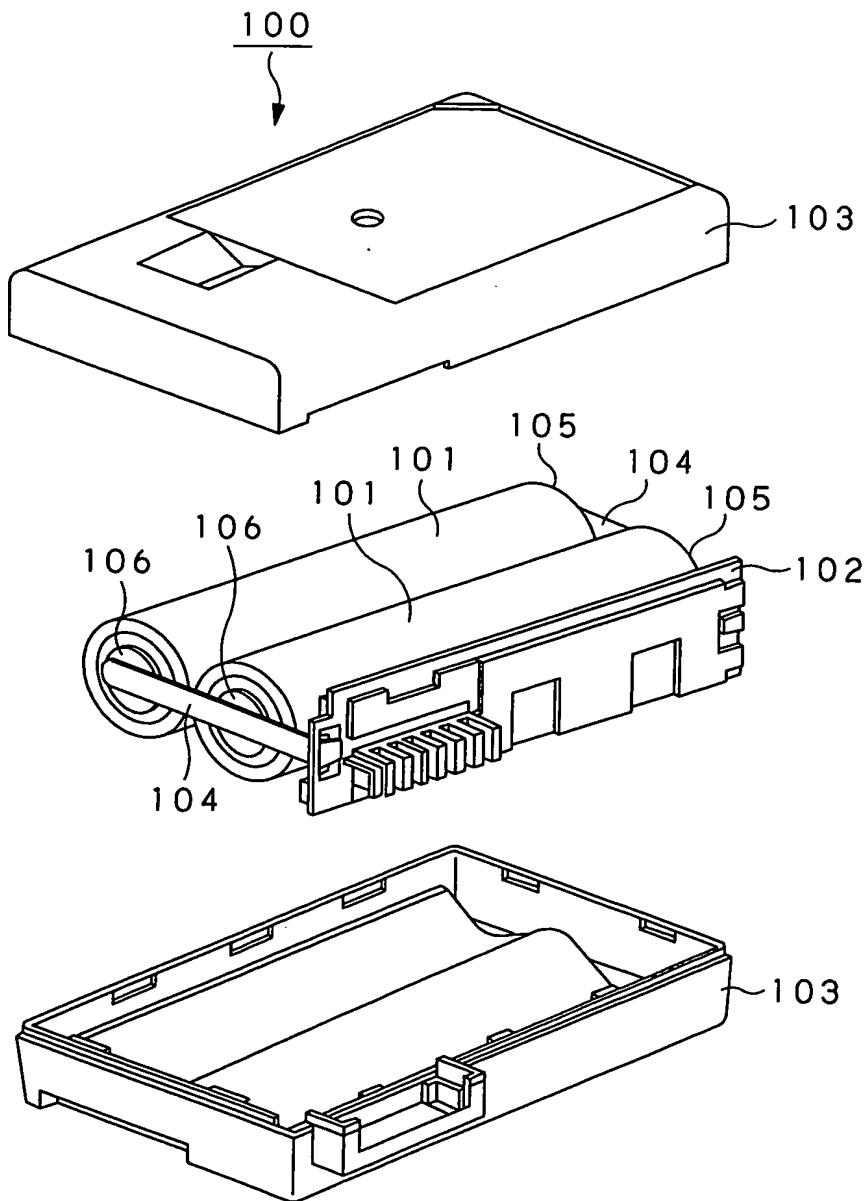


FIG. 1

2/15

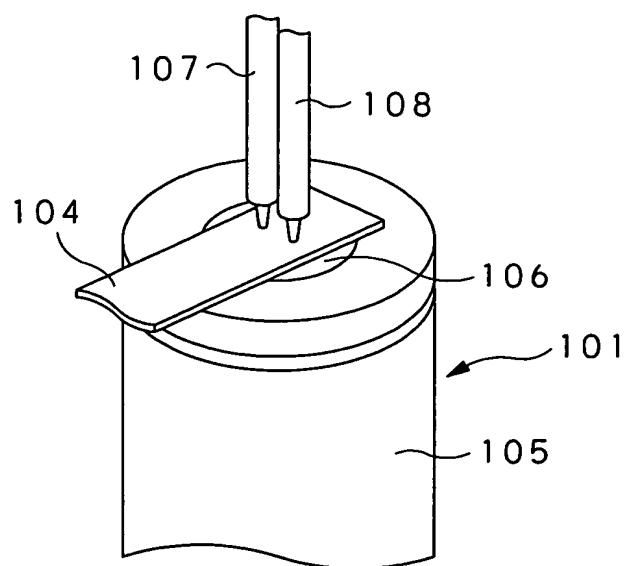


FIG. 2

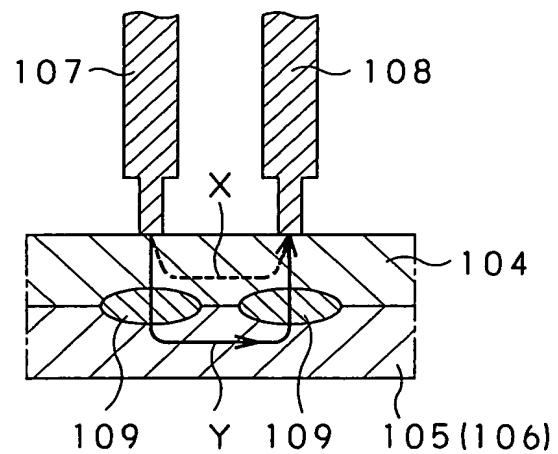


FIG. 3

3/15

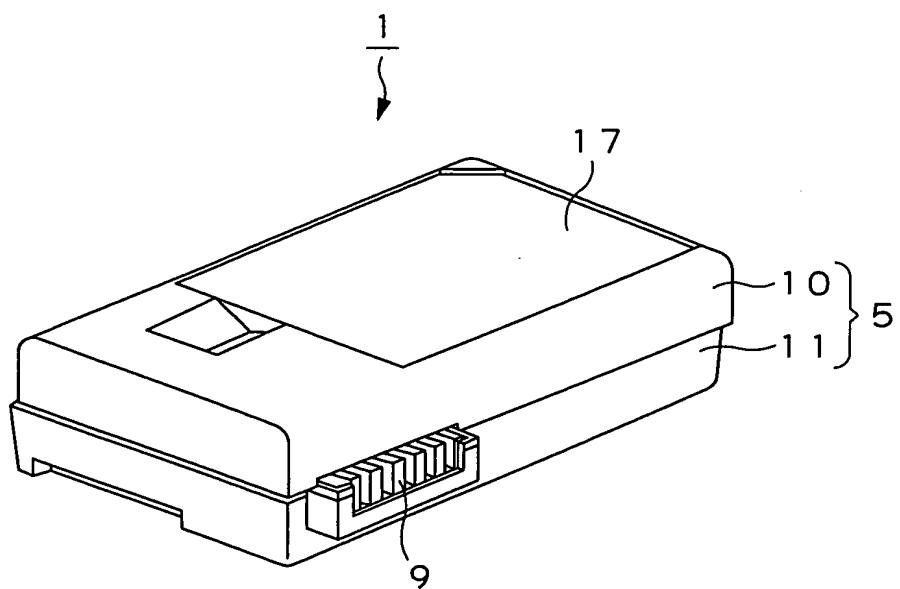


FIG.4

4/15

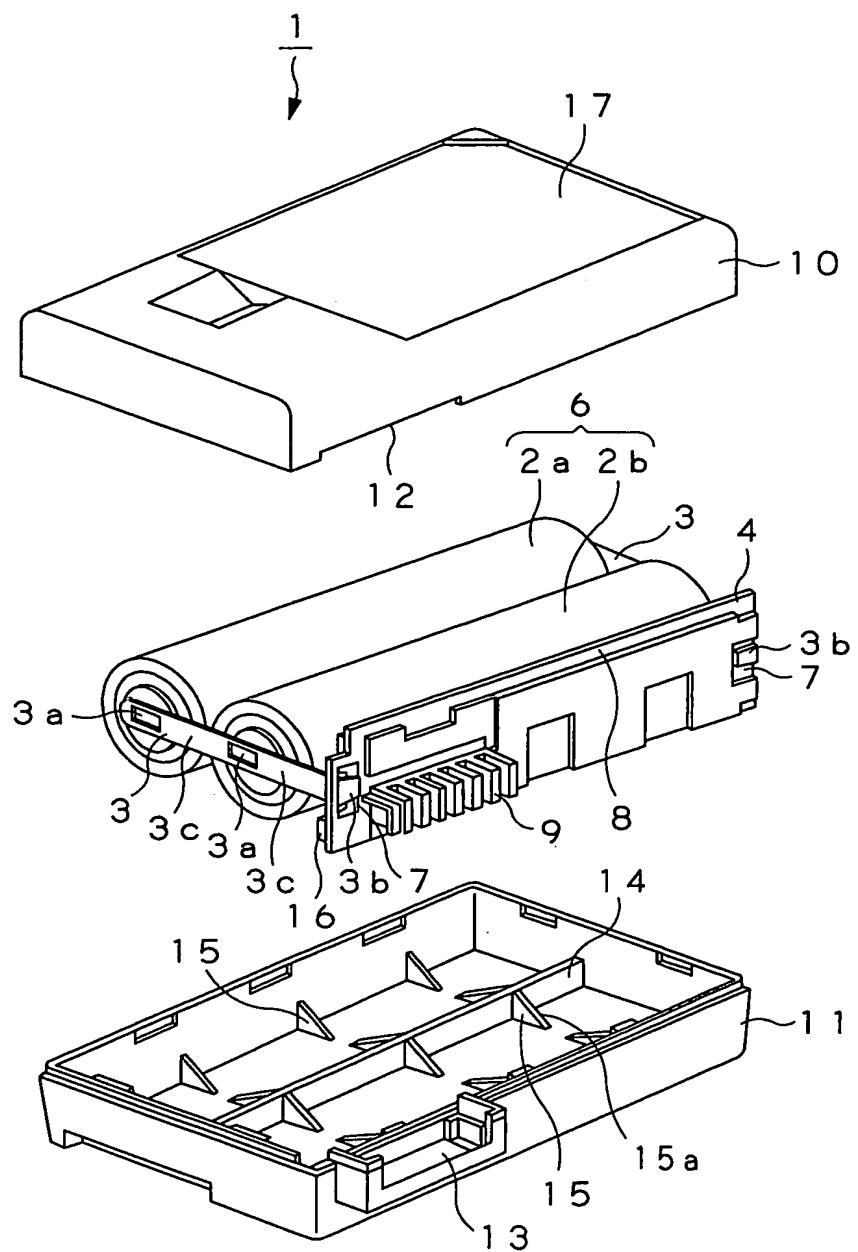


FIG. 5

5/15

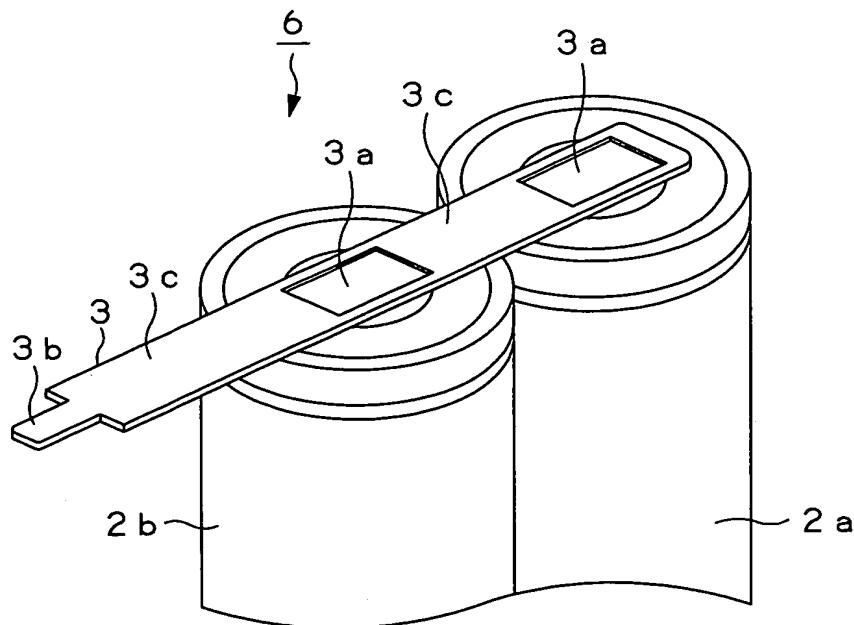


FIG. 6

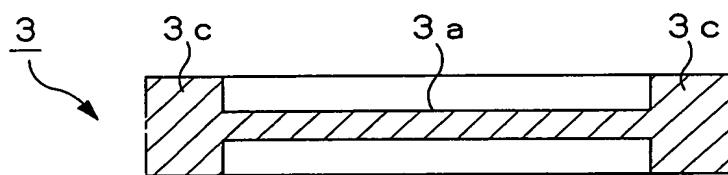


FIG. 7

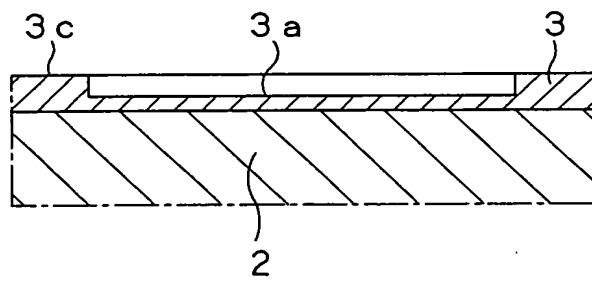


FIG. 8

10/542959

Rec'd PCT/PTO 21 JUL 2005

6/15

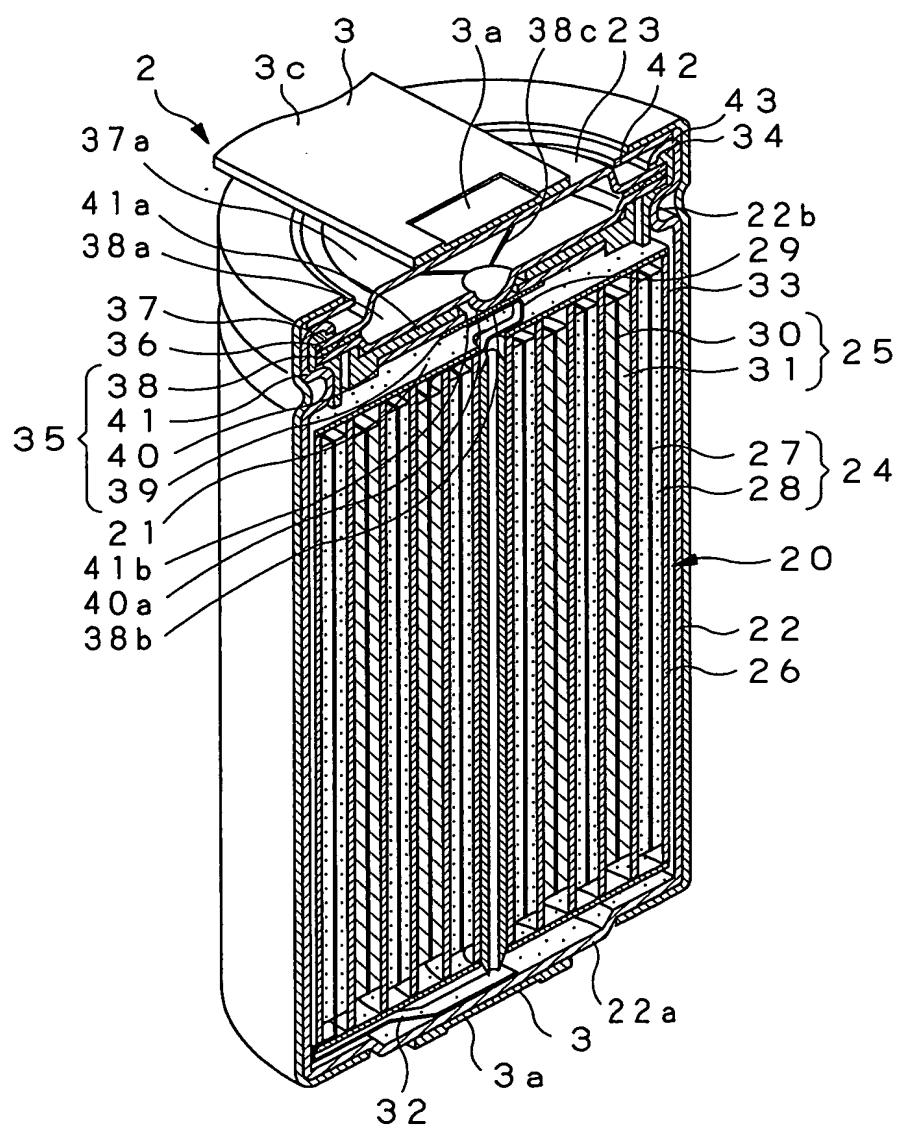


FIG. 9

7 / 15

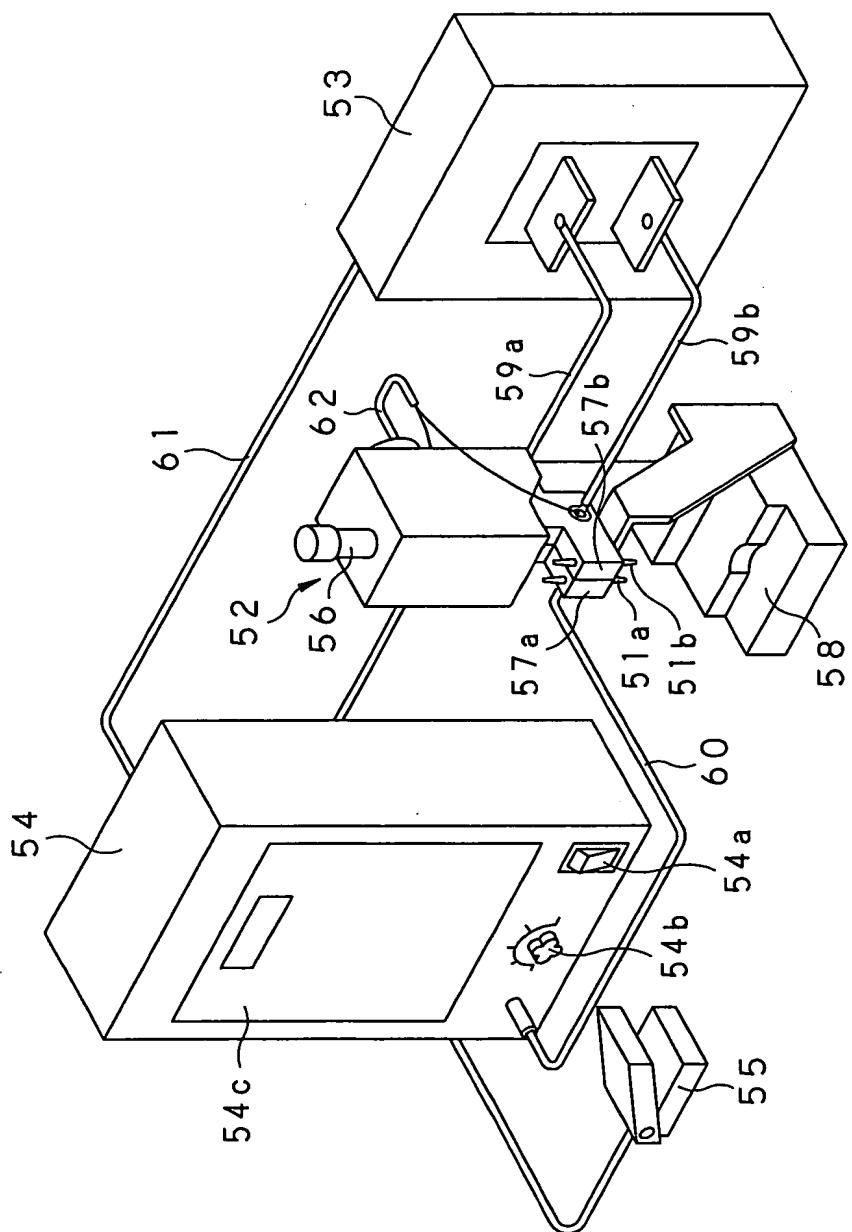


FIG. 10

8/15

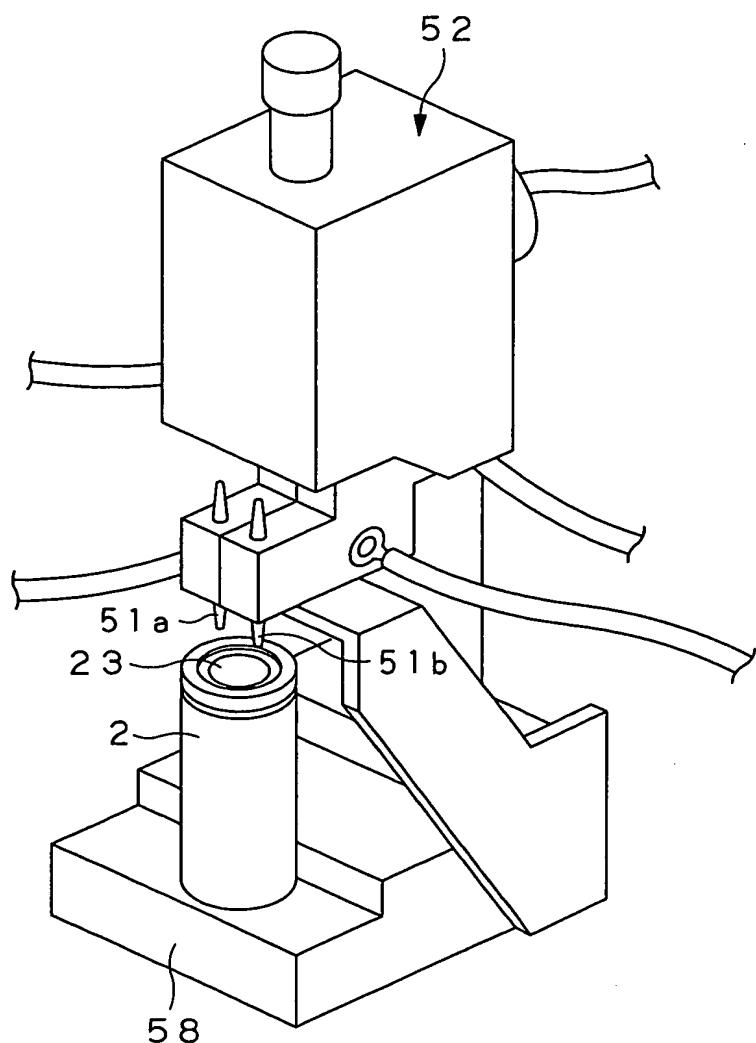


FIG. 11

9/15

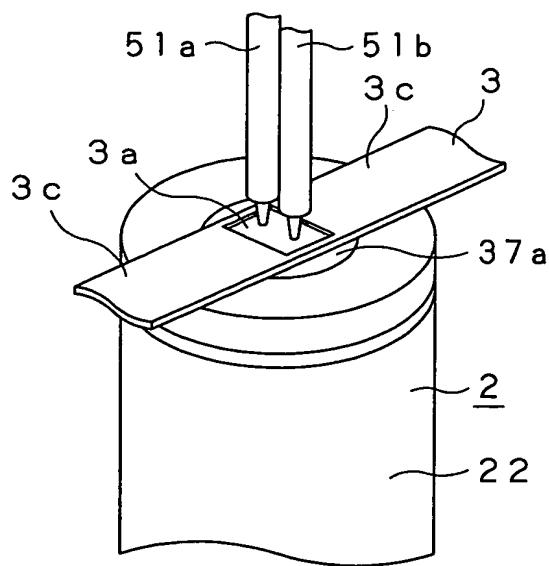


FIG. 12

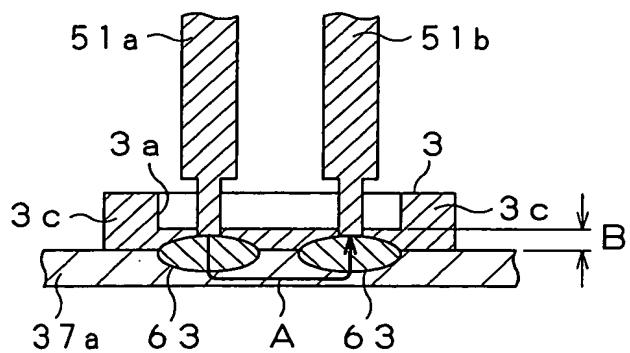


FIG. 13

10/15

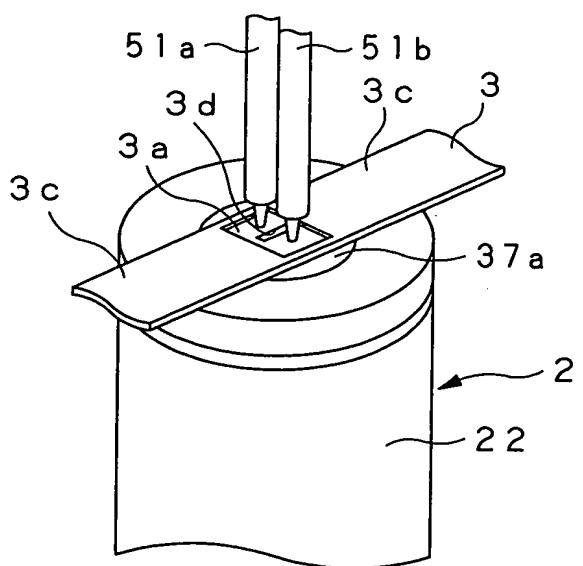


FIG. 14

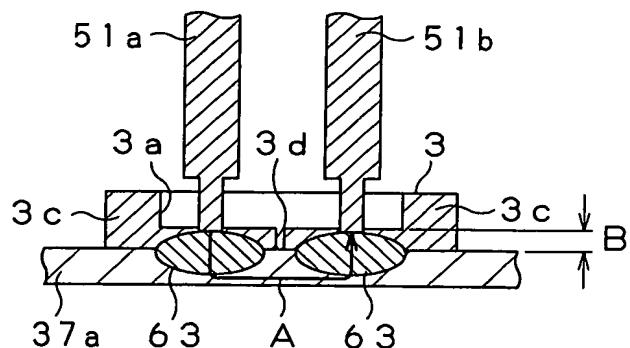


FIG. 15

11/15

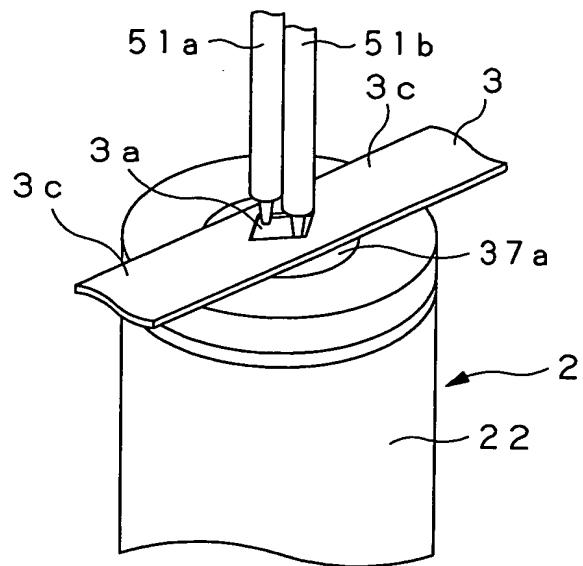


FIG. 16

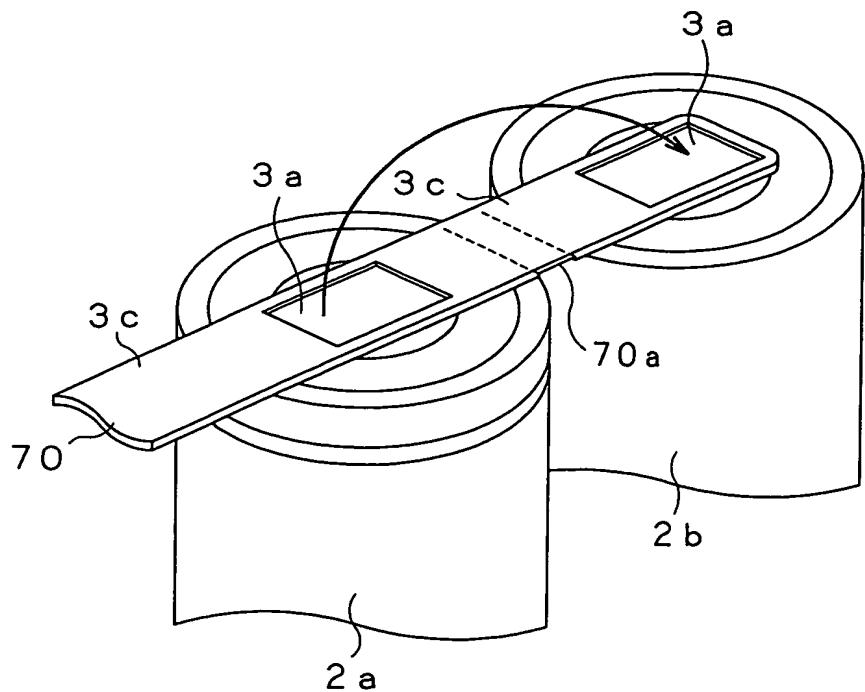


FIG. 17

12/15

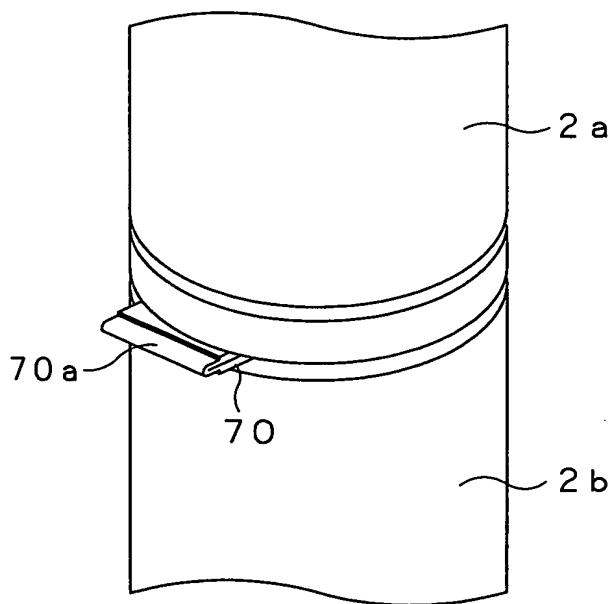


FIG. 18

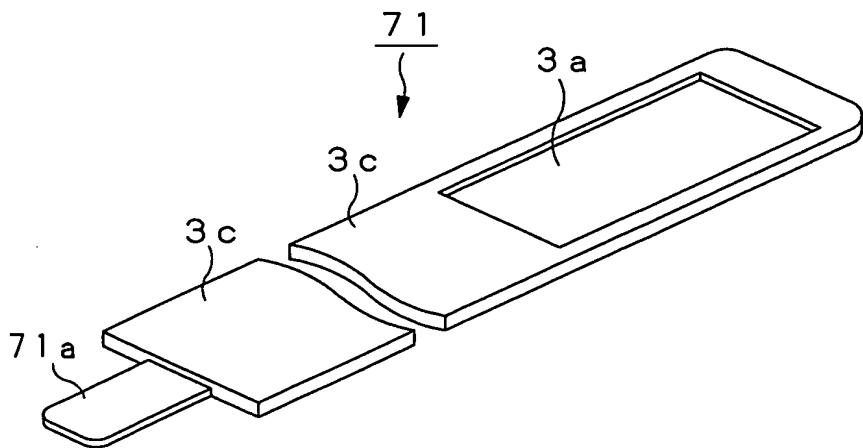


FIG. 19

13/15

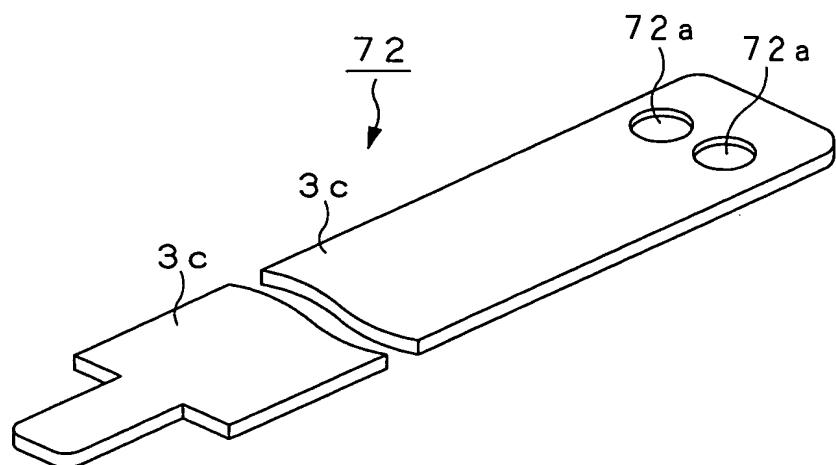


FIG. 20

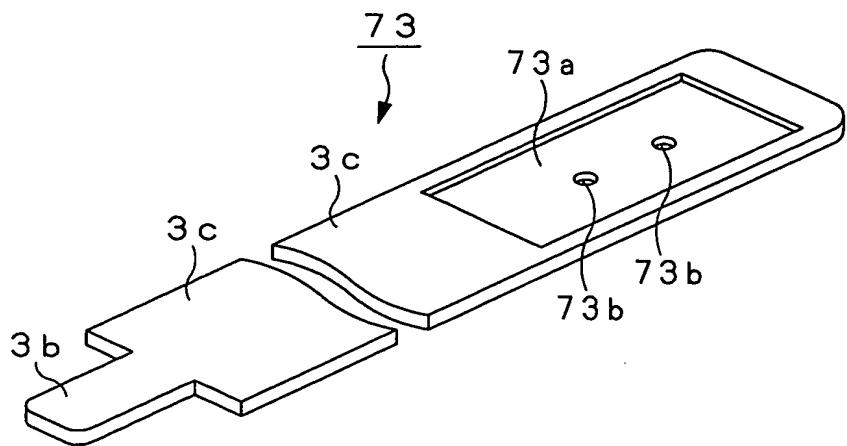


FIG. 21

14/15

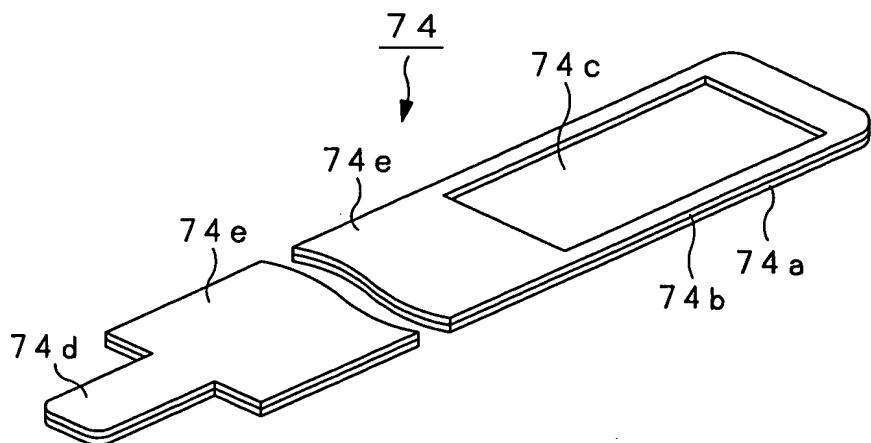


FIG. 22A

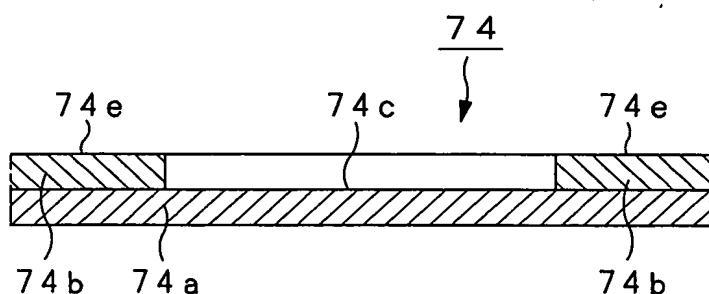


FIG. 22B

15/15

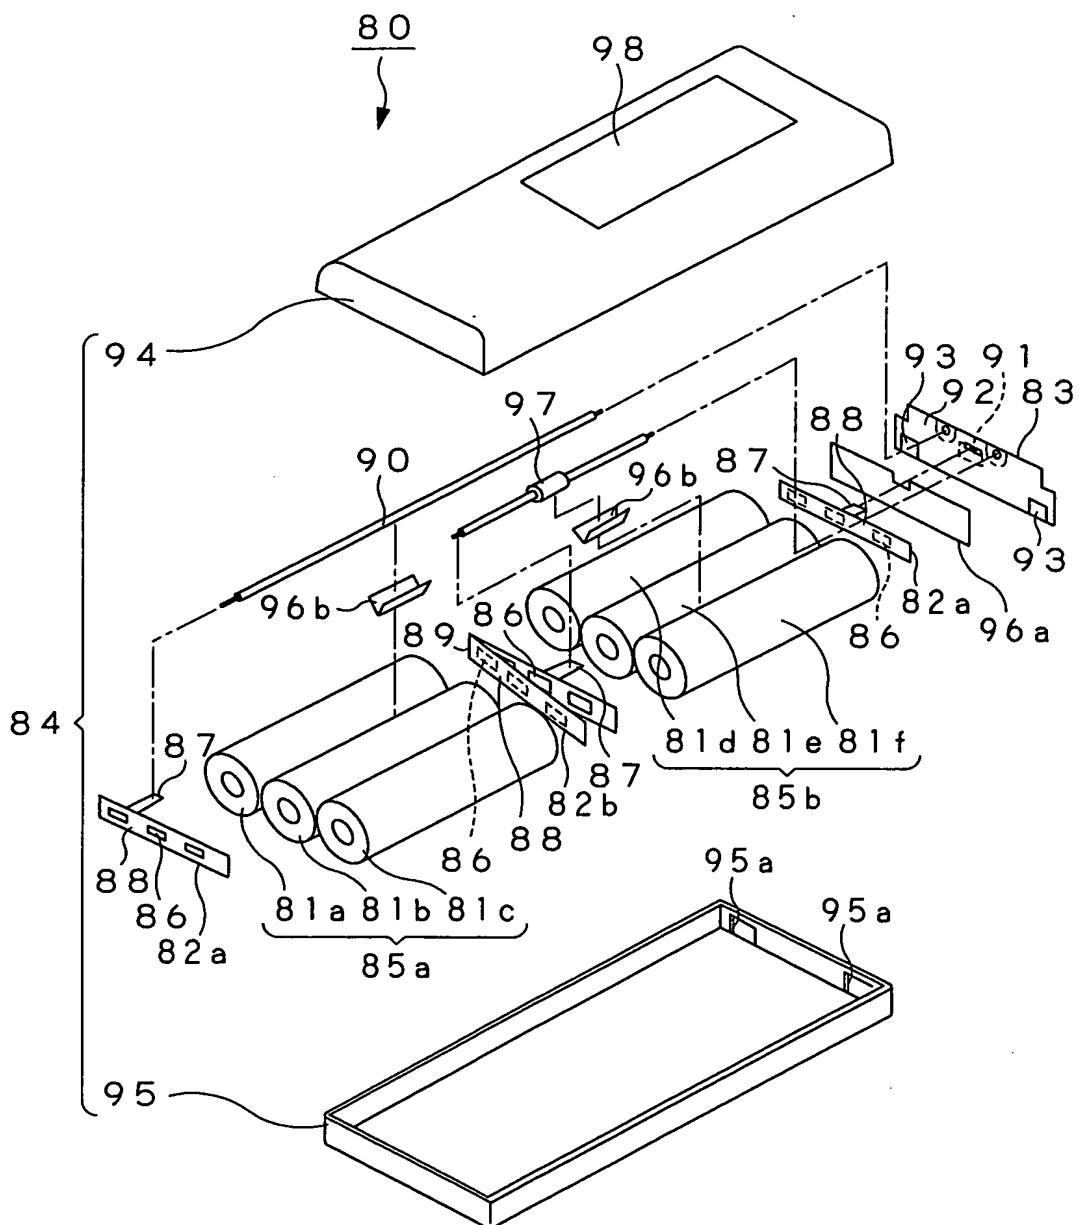


FIG.23